

THERMOACOUSTIC ANALYZER FOR WATER CONTENT DETECTION IN HYDROCARBON EMULSION

Tariq M. Younes, Mohammad A. Al-Khedher* & Mohammad A.K. Alia
Al-Balqa Applied University, Faculty of Engineering Technology
Mechatronics Engineering Department, PO Box 15008, Amman, 11134, Jordan
*Email: moh.alkhedher@fet.edu.jo

ABSTRACT

Water detection in hydrocarbon emulsions represents a serious challenge in petroleum production industry. In this paper, a systematic and an applicable method of water detection in hydrocarbon emulsion is achieved using thermoacoustic effect. The study focused on sensing the presence of water in kerosene using the established correlation between the content of hydrocarbon emulsion and the characteristics of the acoustic wave generated by inundation of a heated rod in the emulsion. This approach was tested experimentally and showed that the produced acoustic signal can be utilized as an informative parameter in quality control schemes of petrochemical oil products.

Keywords: *thermoacoustic, water-in-oil detection, hydrocarbon emulsion, acoustic-wave generation, thermal conductivity.*

1. INTRODUCTION

Thermoacoustics (TA) refers to the physical phenomenon that heat can generate and amplify a sound wave and vice versa. The generation of a stress wave or sound is produced as a consequence of thermal expansion induced by temperature variation. Thermoacoustic technology uses high amplitude acoustic waves in pressurized gas to transfer heat, it also uses temperature difference to induce sound. Recent development and applications of TA systems are mainly based on the work of Rott [1, 2], Steven Garrett and Greg Swift [3], who developed linear thermoacoustic models. Temperature oscillations associated with acoustic waves in fluids allowed the construction of thermoacoustic engines and refrigerators through contact of fluid with surfaces having high heat capacity. Recently, researchers have focused on investigating the potential of utilizing thermoacoustic phenomena in sensing techniques [4, 5]. This paper focuses on sensing the presence of water in oil using oscillatory heat exchange process to detect water content percentage in hydrocarbon fuel. This is achieved through acoustic wave generation by thermal excitation of small regions [6]. In this approach, the key factor contributing to acoustic wave generation is thermal expansion of material and its interaction with volume dilation associated with the acoustic field of receiving transducer.

2. WATER DETECTION IN HYDROCARBON EMULSIONS

Detection of water content in oil products is a significant indicator of oil monitoring procedures as water in oil appears as a hydrocarbon emulsion. Although, several techniques are available to determine water level in hydrocarbon emulsions, they require laboratory equipments to provide accurate and reliable data. Therefore, these procedures are time consuming and not practical for field work, where instant measurement is crucial for management of effective processing.

A well established method for detecting water is using special pastes which alter color on contact with water [7], such as Kolor Kut modified water finding paste or VECOM water finding paste. In literature, one can find a range of efforts in detecting water contamination in gasoline, such as addition of methylen crystal [8], which turns emulsion blue if contaminations existed. Other work suggested detection of water in petroleum products by exposing oil to a substance which is chemically inert. This substance interacts with water to produce gas, and the produced gas is measured by displacement of liquid from a closed vessel [9]. The main drawbacks of this method are complexity and large measurement duration of approximately 3 minutes.

Recently, acoustic research brought much attention to the fields of transducers and devices, which are the basic blocks of laboratory analyzers and measurement systems, such as: gas detectors [10, 11] and temperature detectors [12]. The design of these detectors is based on the measurement of one or more parameters of acoustical characteristics in the domain of interest. Researchers have proposed velocity measurement of sound transmission in the fluid stream [US. Pat. No 4,236,406 and 4,080,837], however, the presence of gas in the stream can affect the measurement. In [U.S. patent No 4,573,346], the volume of water and oil in a stream was determined by consecutive measurement of upstream and downstream sound velocity using a pair of sonic flow meters [13], the resulting data will yield both flow rate and concentration of water in oil. Such a technique is relatively complicated and expensive.

A common method of water detection in petroleum industry is chromatography [14, 15]. Chromatographs are used to give quantitative and qualitative analysis of gases and vapors. However, it is impractical to maintain a chromatograph in non laboratory zone. Gas chromatography is mainly used at early stages of quality control procedures in oil production, whereas the content of oil products may be contaminated as a result of oil storage or during transportation.

Therefore, this research is directed towards the investigation and utilization of a practical method for detecting, monitoring and measuring of water content in hydrocarbon emulsion, and/or detection of oil in water.

3. THERMOACOUSTIC DETECTOR

The operation of this detector is based on the fact that when heat diffuses in the emulsion by the heated rod, a mechanical stress arises, which causes the generation of the acoustic wave whose properties are determined by the characteristics of the medium, i.e. the emulsion thermal expansion forms the acoustic signal [16].

The heat source determines the pressure (P) in an acoustically homogeneous medium at time t and position r as: [17, 18]

$$\nabla^2 P(r, t) - \frac{1}{v_s^2} \frac{\partial^2 P(r, t)}{\partial t^2} = -\frac{\beta}{C_p} \frac{\partial Q(r, t)}{\partial t} \quad (1)$$

Where: β is thermal coefficient of volume expansion, v_s is speed of sound, C_p is the specific heat capacity at constant pressure, and Q is thermal energy per unit time and unit volume.

Assuming the change in volume is negligible, the solution of equation (1) under thermal and stress confinement, subject to zero-initial conditions: [19]

$$P = \frac{\beta v_s^2}{C_p} Q_{abs} = \Gamma Q_{abs} \quad (2)$$

Where: Q_{abs} is the absorbed energy by unit volume of the emulsion. The expression of $\beta v_s^2 / C_p$ represents the Grüneisen parameter (Γ) is a dimensionless factor that is proportional to the fraction of thermal energy converted into mechanical stress; which is related to the thermal and bulk properties of the emulsion. Grüneisen parameter equals to 0.11 for water at 100°C and 0.15-0.2 for hydrocarbon liquids.

Equation (2) demonstrates that the thermoacoustic pressure P is dependent on emulsion characteristics, it varies based on the reaction to changes in emulsion composition including: β , Γ and Q_{abs} at constant temperature [20, 21].

Therefore, the Grüneisen parameter determines the thermoacoustic-conversion efficiency in the emulsion, which is three times larger for water than gasoline [22]. Thus, in practice, the measured acoustic pressure signal generated can be used to monitor the emulsion composition at constant-temperature environment.

4. EXPERIMENTAL SETUP

The proposed sensing method is based on the established correlation between the content of hydrocarbon emulsion and the parameters of generated acoustic wave resulted by inundation of a heated rod in the emulsion.

The system components of TA sensing apparatus are shown in figure 1. Initially, mixing of emulsion was done through consistent shaking. To validate suggested procedure, the mixture was tested in glass, plastic and stainless flasks. Flasks volumes were 1000ml, 500ml, 400ml, 300ml, 200ml and 100ml. The temperature of inundated rod was 100°C and 150°C. The mixture volumes were 100ml, 200ml and 300ml. The acoustic wave is retrieved using a sensitive hydrophone linked to a computer for signal processing.

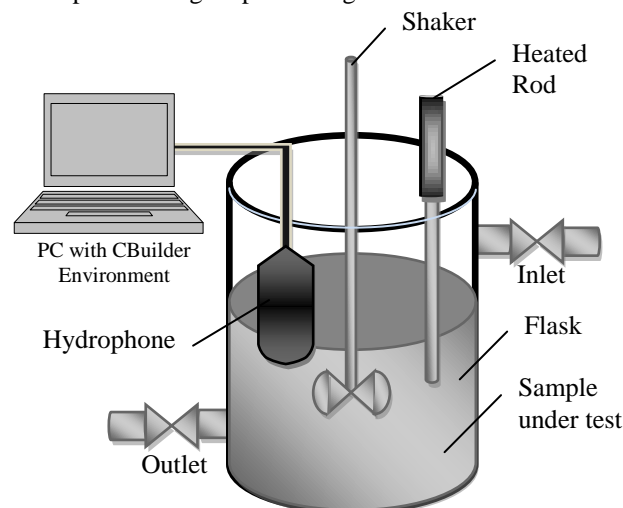


Figure 1: The experimental set-up schematic for water content detection.

In order to study the produced acoustic signal, the signal is analyzed using a customized program under CBuilder-5 environment, it continuously measures the frequency of generated sound signal. The measured frequency which is displayed on a chart recorder yields the desired information about water content in hydrocarbon emulsion.

To investigate the correlation between water content and acoustic wave frequencies, figure 2, the area of acoustic signal peaks (the peak of the basic harmonic) is estimated, this method is frequently implemented in chromatography [23].

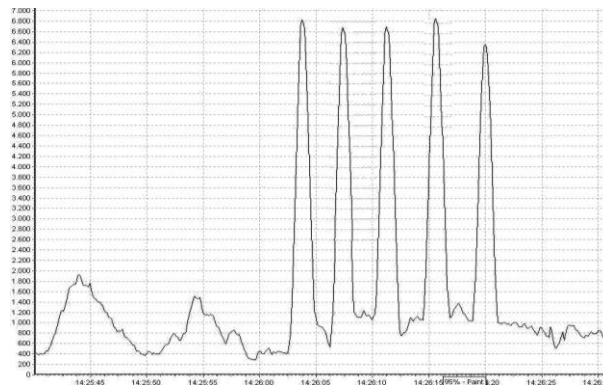


Figure 2: Peaks of acoustic signal for plastic flask at 150 °C, 100ml, 95% kerosene.

Samples are prepared in steady still conditions so that sound resulted by evaporation will not affect the measurements, also consistent temperature should be preserved throughout the procedure.

5. TESTING THERMOACOUSTIC DETECTOR

In order to evaluate the proposed technique and to investigate the relationship between composition and thermoacoustic pressure, multiple water-in-emulsion percentages are tested to estimate the average frequencies of acoustic peaks for different flask types and emulsion volumes as shown in figures 3-5.

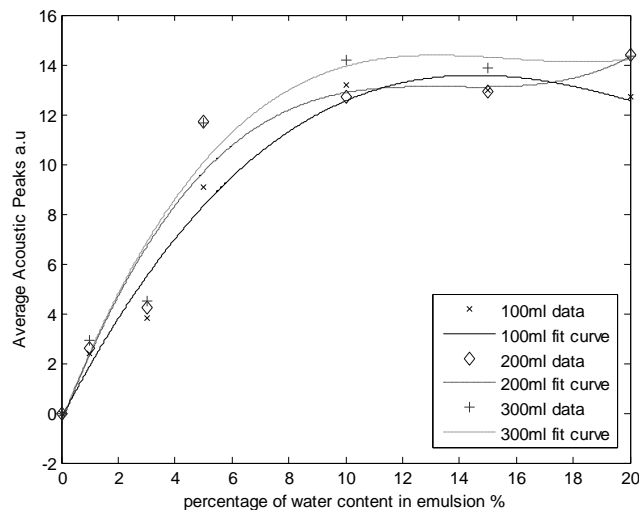


Figure 3: Average frequencies of acoustic peaks with glass flask at 100°C, emulsion volumes: 100, 200, 300 ml.

The average frequency of the acoustic peaks is curve-fitted by a third order polynomial function. The main factors which may affect the generated sound signal are: flask material, heated-rod temperature and volume of mixture. It was found that the temperature variation has a significant impact on the area under the acoustic curve. As shown in figures 3, using different mixture volumes in the same flask has no significant effect on the peaks area of the acoustic wave.

The flask material has a clear effect on peaks area of the sound signal. The type of flask material defines the behavior of produced acoustic signal which depends on the acoustic impedance Z [24]. Z is a characteristic parameter for each medium: $Z_{\text{air}} \approx 4.310^{-4} \text{ Pa}\cdot\text{sm}^{-1}$, $Z_{\text{water}} \approx 1.5 \text{ Pa}\cdot\text{sm}^{-1}$, $Z_{\text{steel}} \approx 45 \text{ Pa}\cdot\text{sm}^{-1}$.

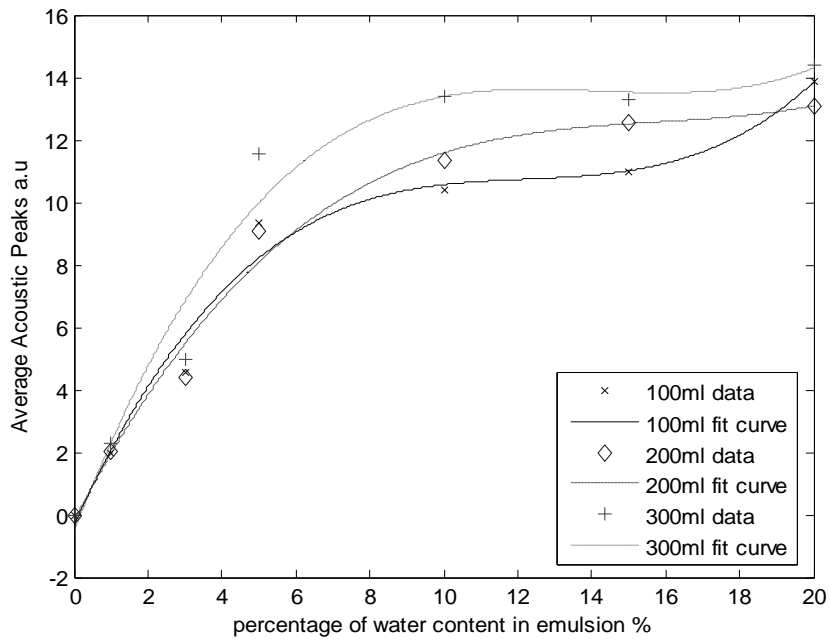


Figure 4: Average frequencies of acoustic peaks with plastic flask at 100°C, emulsion volumes: 100, 200, 300 ml. As shown in figure 5, using a stainless steel flask produces better consistent measurements for various emulsion compositions and flask sizes.

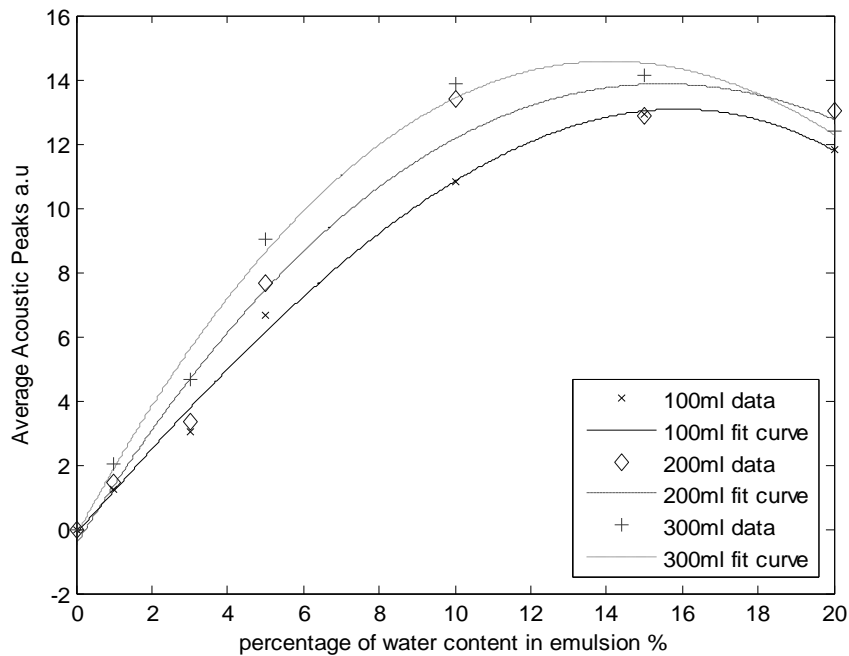


Figure 5: Average frequencies of acoustic peaks with stainless steel flask at 100°C, emulsion volumes: 100, 200, 300 ml. Based on these experimental results, this technique is recommended to detect water-in-oil with percentages of 10% or less. To study the effect of flask sizes on the acoustic signal, shown in figure 6, sizes 100ml, 200ml and 300ml were used in the procedure. As seen the flask size has no effect on the acoustic signal when water content is below 10% of the emulsion.

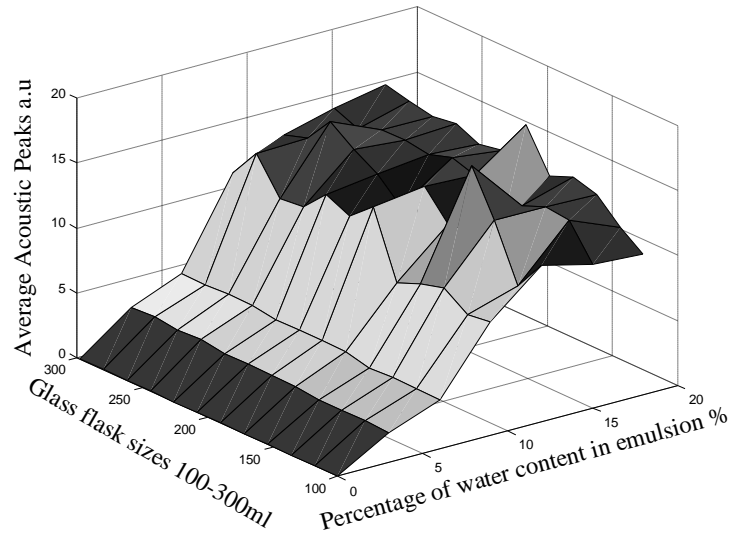


Figure 6: Average acoustic peaks for various glass flask sizes 100-300ml, with different percentages of water content in the emulsion.

Furthermore, several experimental tests were performed to study the influence of using different materials for the flask. As shown in figure 7, the acoustic signal is proportional to the water content under 10% of emulsion with no significant effect of material used.

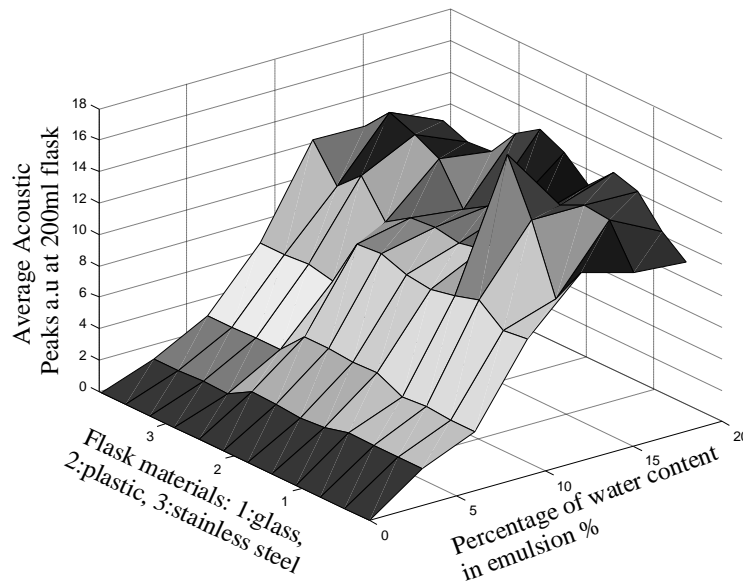


Figure 7: Average acoustic peaks for different Flask materials: 1: glass, 2: plastic, 3: stainless steel, with different percentages of water content in the emulsion.

Based upon these results, this experimental procedure, to use TA principle to detect the water content in hydrocarbon emulsion, established a practical method to monitor water-in-oil in industrial application.

6. CONCLUSIONS

Detection of water content in hydrocarbon emulsion is proposed using the application of a TA-based technique. The experimental results revealed that the generated acoustic signal is related to the properties of the tested hydrocarbon emulsion. The tested thermoacoustic detector demonstrated a sufficient level of precision to sense water-in-oil content if less than 10%. This general approach can be utilized in different quality control tests.

7. REFERENCES

- [1]. Rott N 1969 Damped and thermal driven acoustic oscillations in wide and narrow tubes *Z. Angew. Math. Phys.* **20** 230-43
- [2]. Rott N 1980 Thermoacoustics *Adv. Appl. Mech.* **20** 135-75
- [3]. Swift G W 1988 Thermoacoustic engines. *J. Acoustic. Soc. Am.* **84** 1145-80
- [4]. Ku G, Fornage B D, Jin X, Xu M H, Hunt K K and Wang L H V 2005 Thermoacoustic and photoacoustic tomography of thick biological tissues toward breast imaging *Technol. Cancer Res. Treat.* **4**(5) 559–65
- [5]. Pramanik M, Ku G, Li C H and Wang L H V 2008 Design and evaluation of a novel breast cancer detection system combining both thermoacoustic (TA) and photoacoustic (PA) tomography *Med. Phys.* **35**(6) 2218–23
- [6]. Kino G S and Stearns R G 1985 Acoustic wave generation by thermal excitation of small regions *Appl. Phys. Lett.* **47**(9) 926-8
- [7]. Iqbal M, Morel O and Meriaudeau F A 2009 Survey of outdoor water detection *The 5th International Conference on Information & Communication Technology and Systems (ICTS) Indonesia*
- [8]. Guven K C and Gezgin T 2004 The water detection in gasoline and its hydrocarbon contents *J. Black Sea Mediterr. Env.* **10** 61-70
- [9]. Pedersen A B 1977 Detection of water in oil, US patent 4089652
- [10]. Younes T 2003 Acoustic detector for gas chromatography, Russian Federation Patent 33233
- [11]. Younes T 2003 Acoustic detector of gases and vapors, Russian Federation Patent 33822
- [12]. Alia M A K and AlMograbi T 2007 Investigation of An Acoustic Temperature Transducer and its Application for Heater Temperature Measurement *Am. J. Appl. Sci.* **4**(5) 294-9
- [13]. Zachrias E M Jr 1986 Method of measuring the composition of an oil and water mixture, US Patent 4573346
- [14]. Senn R B and Johnson M S 1987 Interpretation of gas chromatography data in subsurface hydrocarbon investigations *Ground Water Monit. Rev.* **7**(1) 58-63
- [15]. Acqua R D, Egan J A and Bush B 1975 Identification of petroleum products in natural water by gas chromatography *Environ. Sci. Technol.* **9**(1) 38–41
- [16]. Srivastava R K, Dhabal R L, Suman B M, Saini A and Panchal P 2006 An estimation of correlation on thermo-acoustic properties of mineral wool *J. Sci. Ind. Res.* **65** 232-6
- [17]. Guo B, Li J, Zmuda H and Sheplak M 2007 Multifrequency microwave-induced thermal acoustic imaging for breast cancer detection *IEEE Trans. Biomed. Eng.* **54**(11) 2000–10
- [18]. Lou C and Xing D 2010 Temperature monitoring utilising thermoacoustic signals during pulsed microwave thermotherapy: A feasibility study *Int. J. Hyperther.* **26**(4) 338–46
- [19]. Xu Y, Wang LV, Ambartsoumian G and Kuchment P 2004 Reconstructions in limited-view thermoacoustic tomography *Med. Phys.* **31** 724–3
- [20]. Aktas M K and Farouka B 2004 A Numerical Study of The Generation and Propagation of Thermoacoustic Waves in Water *Phys. Fl.* **16**(10) 3786-94
- [21]. Toubal M, Asmani M, Radziszewski E and Bertrand N 1999 Acoustic measurement of compressibility and thermal expansion coefficient of erythrocytes *Phys. Med. Biol.* **44** 1277-87
- [22]. Ozoe H, Sato N and Churchill S W 1980 The Effect of Various Parameters on Thermoacoustic Convection *Chem. Eng. Commun.* **5** 203-21
- [23]. Felinger A 1998 *Data Analysis and Signal Processing in chromatography* (Amsterdam: Elsevier Science, Handling science and technology, Vol. 21) 192-3
- [24]. Pallas-Areny R and Webster J G 2001 *Sensor and signal conditioning* 2nd edition (New York: John Wiley and sons)